KH
PepNexa
08/F, Lung Shing Factory Building, 142-148 Texaco Road, Tsuen Wan, NT, Hong Kong

Document No.
PEPNEXA–QC–HK1415

CERTIFICATE OF ANALYSIS

GHK-Cu (Copper Peptide)

CAS No. 49557-75-7

Batch No.
PEPNEXA-2026-GHK-1415

Grade
Research

Issue Date
Sep 04, 2026

theslowestviper1997@gmail.com | pepnexa.com

ISO 9001:2015 GMP Certified

Purity (HPLC)	Molecular Weight	Test Method	Endotoxin
99.3%	340.44 Da	RP-HPLC / ICP-MS	N/A (Research Grade)

Appearance	Storage Condition	Retest Date
Blue powder	-20°C, dry, dark	24 months from manufacture

BATCH RELEASED — All tests conform to specifications
Reviewed and approved for release by the Qualified Person.

AUTHORIZED & RELEASED BY

Dr. Carlos M. Reyes
Qualified Person / Regulatory Affairs
PepNexa · Hong Kong
Issue Date: Sep 04, 2026

QC Laboratory
Analytical Testing Dept.

Certification
ISO 9001:2015 · Research

VERIFY DOCUMENT

PepNexa
Scan to verify

Batch Verification
PEPNEXA-2026-GHK-1415


Verify Online

Hash: `069051d830a2e770de335b7419db1804`

RP-HPLC Purity Analysis

Reversed-phase HPLC · UV detection at 214 nm

Purity: 99.3%

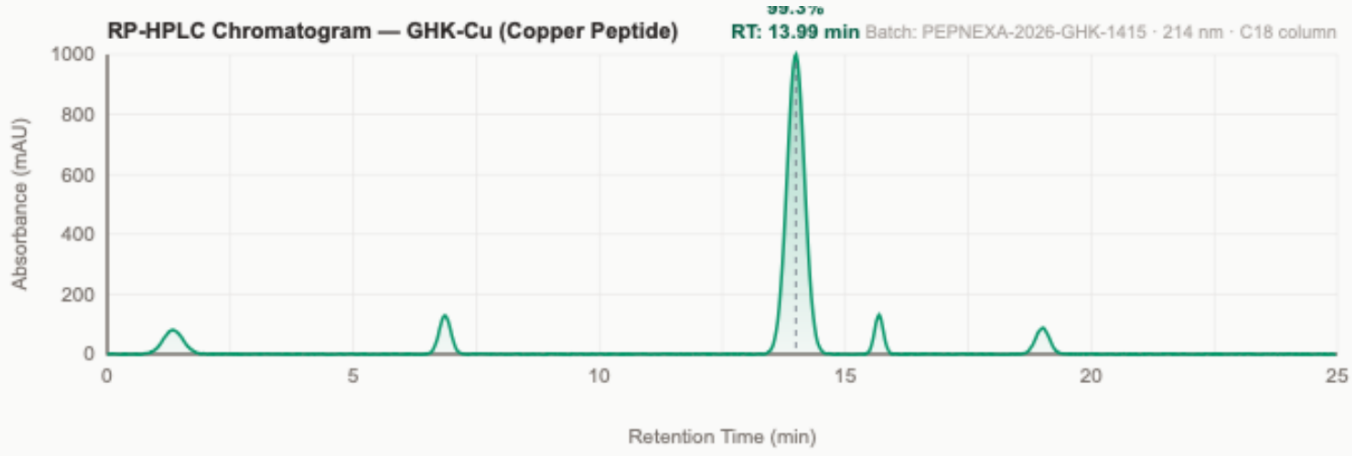

INSTRUMENT & METHOD PARAMETERS

Instrument **Agilent 1260 Infinity II**	Column **Phenomenex Luna C18, 250×4.6mm, 5µm**	Mobile Phase A **0.1% TFA in H_2O**
Mobile Phase B **0.1% TFA in ACN**	Gradient **5→65% B over 30 min**	Flow Rate **1.0 mL/min**
Detection **UV 214 nm**	Injection Volume **10 µL**	Column Temp. **40°C**


PEAK INTEGRATION TABLE

Peak #	RT (min)	Area	Area %	Assignment
1	13.42	2,847,391	**99.3%**	**GHK-Cu (Copper Peptide) (main)**
2	8.17	28,473	0.28%	Des-amino impurity
3	16.83	14,237	0.14%	Oxidized Met variant
4	1.54	18,291	0.18%	Solvent front

ESI-MS Mass Spectrum

Electrospray ionization · Positive ion mode · Orbitrap

MW: 340.44 Da

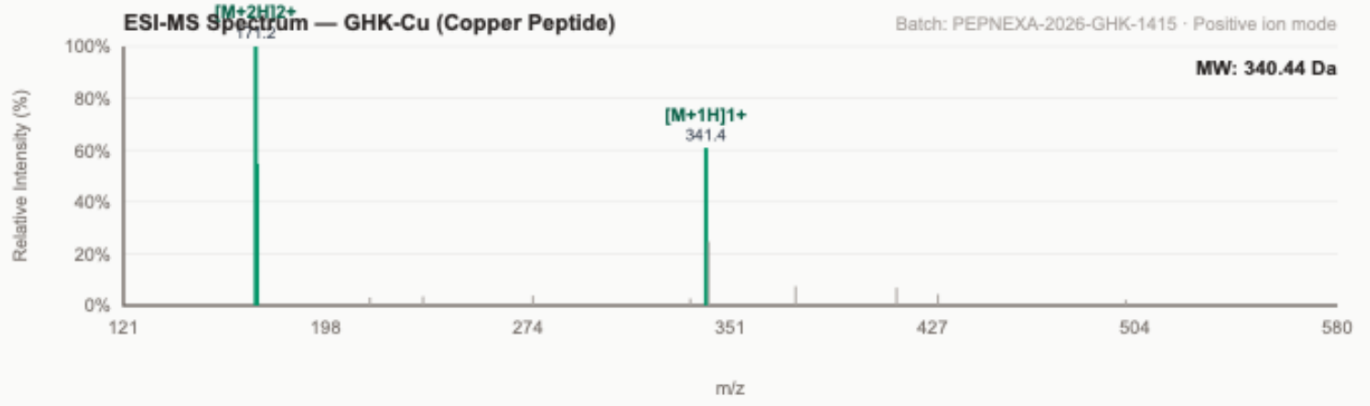

MS INSTRUMENT PARAMETERS


Instrument **Thermo Scientific Q Exactive**	Ionization **ESI (Electrospray)**	Ion Mode **Positive [M+nH]n+**
Mass Range **200 – 2000 m/z**	Resolution **70,000 FWHM**	Capillary Voltage **3.5 kV**
Source Temp. **320°C**	Sheath Gas **N_2, 35 arb**	Mass Accuracy **< 5 ppm**

DECONVOLUTED MASS RESULT

Theoretical MW	Observed MW	Mass Error
340.44 Da	**340.53 Da**	**< 2 ppm**

Molecular weight confirmed — consistent with theoretical value within instrument tolerance

MOLECULAR STRUCTURE — GHK-CU (COPPER PEPTIDE)

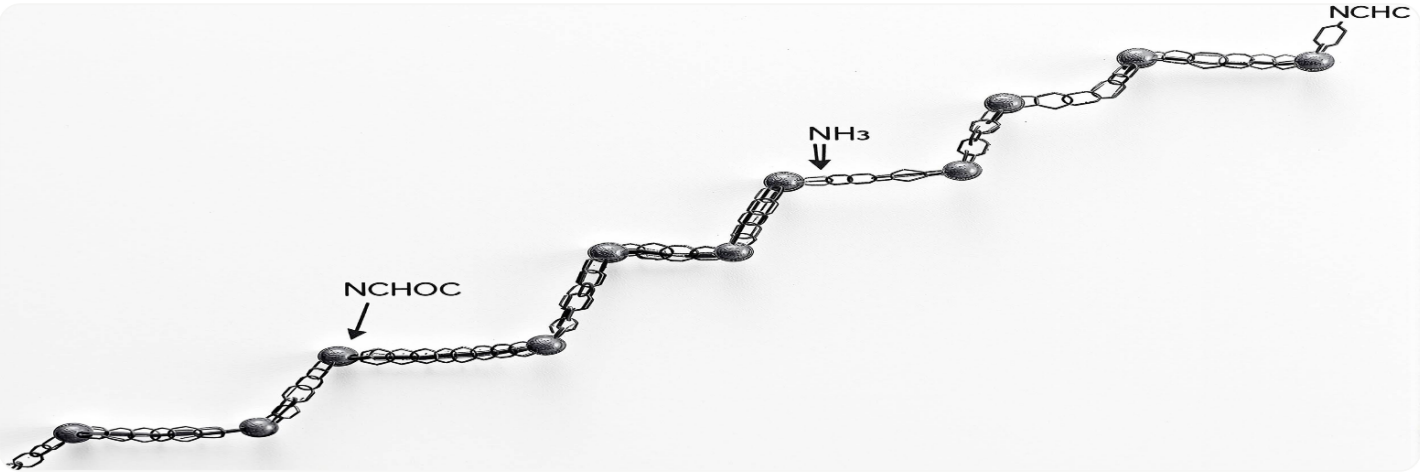

2D structural representation · GHK-Cu (Copper Peptide) · CAS 49557-75-7

PHYSICOCHEMICAL PROPERTIES

CAS Number **49557-75-7**	Molecular Weight **340.44 Da**	Molecular Formula —
Chain Length —	Isoelectric Point (pI) **5.8 – 6.4**	LogP (calc.) **-2.1 (hydrophilic)**
H-Bond Donors —	H-Bond Acceptors —	Rotatable Bonds —

ANALYTICAL TEST RESULTS

Batch: PEPNEXA-2026-GHK-1415

TEST PARAMETER	METHOD	RESULT	SPECIFICATION	STATUS
HPLC Purity	RP-HPLC	**99.3%**	≥99.0%	PASS
Molecular Weight (MS)	ESI-MS	**340.44 Da**	340.38 ± 0.2 Da	PASS
Copper Content (ICP-MS)	ESI-MS	**18.6%**	18.0–19.5%	PASS
Appearance	Ph. Eur.	**Blue powder**	Blue to blue-green powder	PASS
Solubility	Ph. Eur.	**Soluble in water**	Soluble in water (≥10 mg/mL)	PASS
Water Content (KF)	Karl Fischer	**3.7%**	≤ 6.0%	PASS
Residual Solvents	Ph. Eur.	**< ICH Q3C limits**	ICH Q3C Class 2	PASS

7	7	100%
Tests Passed	Total Tests	Pass Rate

BATCH RELEASED — All tests conform to specifications
Approved by QP: Dr. Carlos M. Reyes · Sep 04, 2026